

**ZINGLER-Messtechnik e.K.**  
Seppenser Mühlenweg 11  
21266 Jesteburg–Germany  
Tel.: +49 4181 2197732  
kontakt@zingler-messtechnik.com

datasheet  
thermocouple measuring device  
TH-ME-NiCr-Ni-231-20-7mm

The thermocouple measuring device serves for measuring the temperature of electrically conductive metal surfaces. In particular, the temperature of the metal surfaces, the emission factor pyrometers with largely undefined is, can this unit in Seconds measured.

For this purpose, the measuring device coupled with a hydraulic or pneumatic mechanical transport device.



The probe tips in diameter 7,0 mm are biased by springs and by the hydraulic or pneumatic forward stroke with a spring force of about 28 N against the surface to be measured pressed. The measured value is available immediately after touching the probe tips to the metal surface. The spring path of the probes may be up to 20 mm.

The housing consists of a massive steel pipe with welded flange bolt circle 100 mm. The sensor head is made of aluminum with internal parts of heat-resistant plastic and ceramic as an insulator. The probe tips are open thermocouple wires in NiCr (green)+ and Ni (white)-type K.

For the evaluation of the generated thermal voltage, a special transducer (type 231 with galvanic isolation) is required, which converts the thermal voltage into a standardized output signal 4 ... 20 mA (corresponds to the temperature measuring range) immediately after the delay time when the measuring tip is touched with the metal surface to be measured. Without touch (open measuring tips), the connected measuring transducer goes into the overflow (21 mA = over the measuring range end).



The transmitter can be mounted as a rail mount in a separate housing. We will be pleased to provide you with this measuring transducer. The electrical connection between the two measuring probes and the transmitter must be carried out by means of the provided compensation cable for Type K. ***If, contrary to expectation, this is too short, it may only be extended with the same compensating cable. The ends to be connected are to be clamped in a metallically conductive manner.***

The thermocouple measuring device is suitable for short time temperature measurement of metal surfaces to 600 ° C.




Jesteburg, 30.06.2021, Subject to change



Zingler-Messtechnik e.K. | Seppenser Mühlenweg 11 | 21266 Jesteburg / Germany  
Tel: +49 4181 2197732 | Fax: +49 4181 2197733 | kontakt@zingler-messtechnik.com

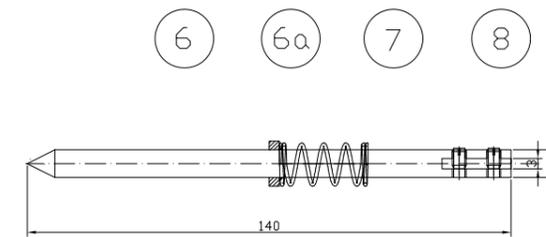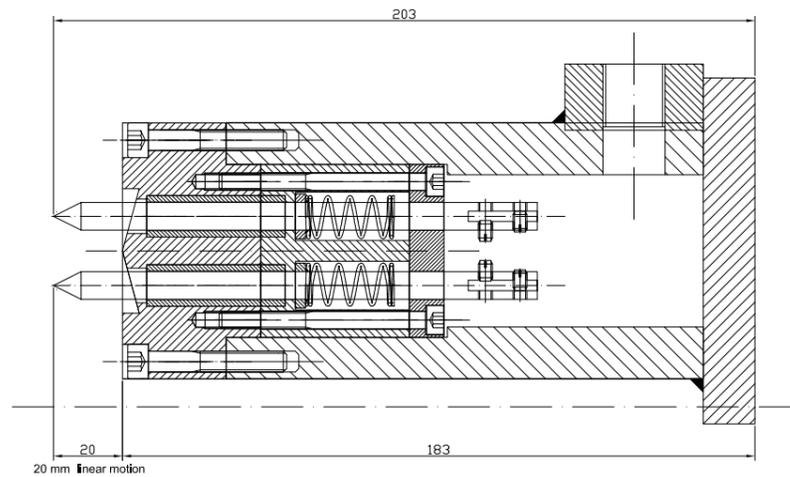



- | pos. | description  |
|------|--|
| 1    | in front part Aluminium  |
| 2    | middle part Ketron Peek 1000   |
| 3    | back part Ketron Peek 1000   |
| 4    | screw M6x40  |
| 5    | screw M5x60  |
| 6    | measuring probe Ni - white - magnetic 7,0mm Ø                        |
| 6a   | measuring probe NiCr + green - nonmagnetic 7,0mm Ø                   |
| 7    | spiral spring D-150C   |
| 8    | ring 13x7x3 mm   |
| 9    | tube 74x15, 138 mm long  |
| 10   | flange 100x100x15 mm,  |
| 11   | ceramic hull alu-oxid Rapal 100<br>dimensions 12 x 7 x 40 mm         |
| 12   | socket in M18x1,5, length 23 mm                                      |
| 13   | for cable entry M18x1,5:<br>cabelgland Dose BORNEO CVKS 18 Z18-06 cr |

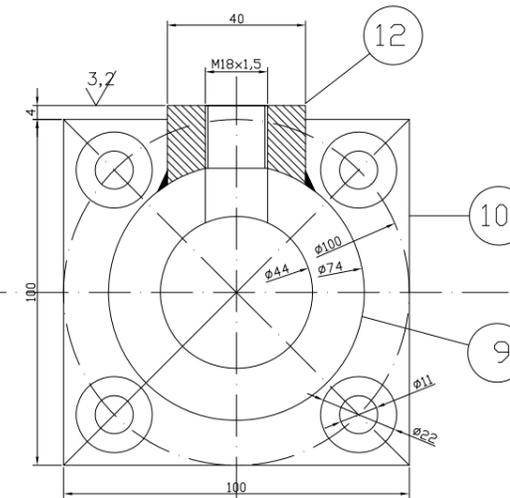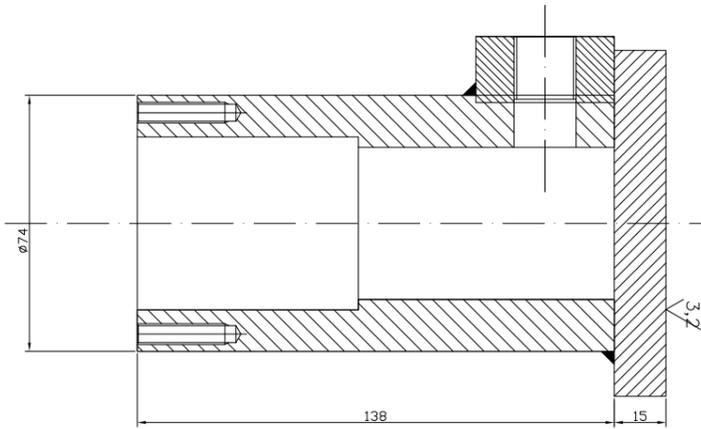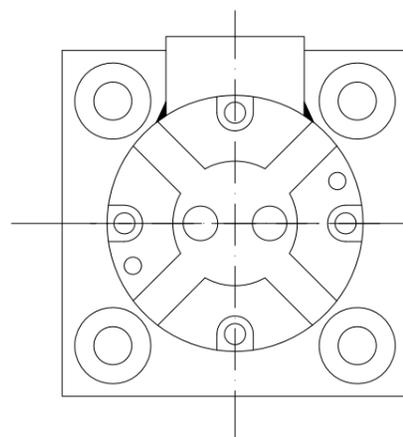

more material:  
 10 m compensating cable,  
 insulation: silicone, fiberglass and  
 galvanized steel wires,  
 wire stranded 48x0,2 mm  
 2 x 1,5 mm<sup>2</sup>, type K, shape: round  
 order.-no.: AGL-1XK-2X1,5SGPR-IEC  
 with standard plug green NiCr-Ni  
 with standard coupling green NiCr-Ni

transmitter type 231 (galv. sep.)  
 for thermocouples type K to analog signal 4...20 mA, range 0...600°C or other,  
 Loop voltage: 24 VDC

Assembly: Cable entry 90° for alignment of the measuring tips

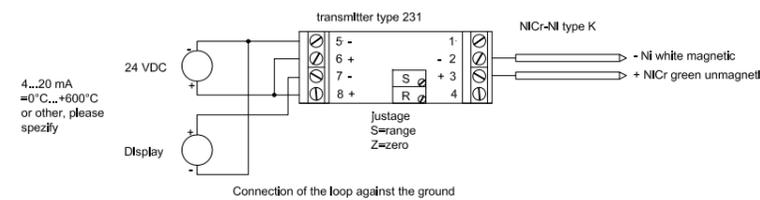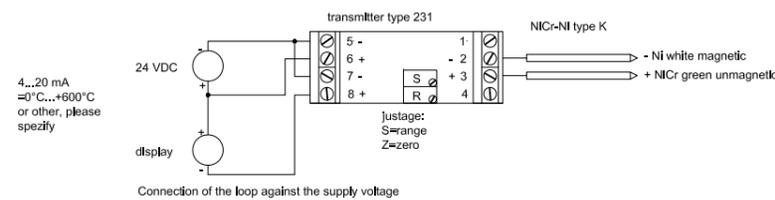


7 mm measured peaks,  
 20 mm linear motion

(Verwendungsbereich)	(Zul. Abw.)	(Oberfl.)	Maßstab 1:2	(Gewicht)
			(Werkstoff, Halbzeug) (Rohteil-Nr) (Modell- oder Gesenk-Nr)	
	Bearb. 30.07.19	Name ZINGLER	TH-ME-NiCr-Ni-231-20-7mm	
	Gepr. 30.07.19	ZINGLER		
	Norm			
	Zingler-Messtechnik e.K. Seppenser Mühlenweg 11 21266 Jesteburg			Blatt
Zust.	Änderung	Datum	Name (Urspr.)	(Ers. f.)
				(Ers. d.)

## LKM231 FOR THERMOCOUPLES


### Analogue galvanically isolated measurement converter for thermocouples to be mounted on 35mm track with a 4..20mA output signal

The LKM 231 is an analogue measurement converter for various thermocouples in accordance with DIN EN 60584 and DIN EN 43710. It converts the temperature-dependent thermoelectric voltage from the sensors into a standard current signal of 4 .. 20 mA. It features galvanic isolation between input and output. The temperature compensation for the reference junction takes place in the actual measurement converter. The measurement converter is supplied with a factory calibration according to customer requirements. You will find further technical data in the instructions for use of the LKM231. Power can be supplied from a voltage source.

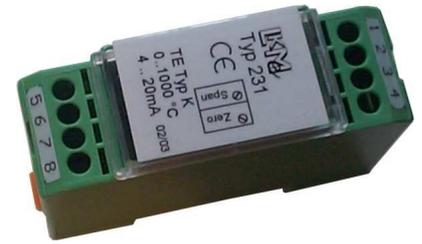


### TECHNICAL DATA

Input:	thermocouples K,J(L),T(U), E,	N, S, B with higher error
Zero:	-200..600°C	depending upon thermocouple
Span:	>200 K	depending upon thermocouple
Linearity error:	<1% FS	depending upon thermocouple
Error of reference junction:	<±0.5°C	
Ancillary voltage:	24VDC ±10%	with security against polarity reversal
Loop voltage:	10..35VDC	polarity - safe
Current consumption:	max. 40mA	
Output:	4..20mA	current loop
Test voltage:	1kV	
Probe break:	>20mA	
Short circuit:	current value for room temperature	
Reaction time:	<0.1s	
TC:	<100ppm/°C	
Operating temperature range:	-25..85°C	
Humidity:	<95%	
Mounting:	35mm rail	
Housing:	EMG25-LG made of polycarbonate	
Dimensions:	75x25x53mm	HxWxD
Type of terminal:	screw clamps	
Clamping range:	0.2..2.5mm <sup>2</sup>	
Weight:	approx. 60g	
Vibration:	5g/10..200Hz	
EMC:	EN 61000-6-3:2001 EN 61000-6-2:2001	Emission and Resistance to interference

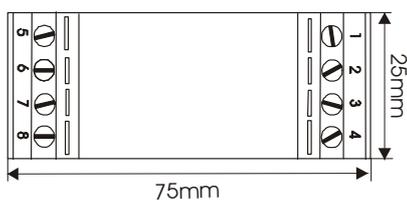


Load resistance

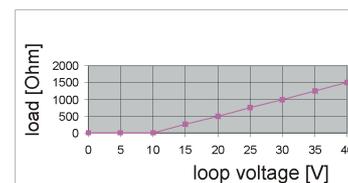

## LKM231 INSTRUCTIONS FOR USE

The Type 231 is an analog transmitter and electrically isolated base mainly for thermocouples. It converts the temperature-dependent thermal voltage linear voltage into a standard current signal of 4...20 mA. The transmitter model 231 is designed for installation in 35 mm DIN rail.

### OPENING THE HOUSING AND LOCATION OF CONTROLS

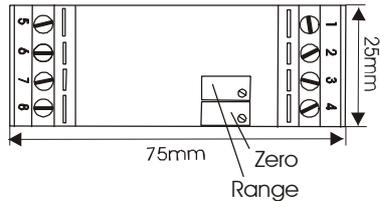

To open the clear view cover this must be carefully pressed inwards on the narrow sides and lifted off. The location of the potentiometers can be seen in the adjacent figure. The potentiometers are protected against inadvertent adjustments. The null point potentiometer can be adjusted to make small corrections. The range potentiometer should be adjusted as little as possible.

### THERMOCOUPLE CONNECTIONS

The plus leg of the thermocouple is connected to terminal 3 of the transmitter and the minus leg to terminal 2.

Color identifiers for compensating leads in accordance with DIN EN 60584

Couple	Type	Sleeve color	Plus leg	Minus leg
Fe-CuNi	J	black	black	white
NiCr-Ni	K	green	green	white
Cu-CuNi	T	brown	brown	white

Color identifiers for compensating leads in accordance with DIN 43713



Couple	Type	Sleeve color	Plus leg	Minus leg
Fe-CuNi	L	blue	red	blue
Cu-CuNi	U	brown	red	brown

Color identifiers for compensating leads in accordance with DIN 43714

Couple	Type	Sleeve color	Plus leg	Minus leg
NiCr-Ni	K	green	red	green

### EXTERNAL CIRCUIT

The output voltage follows the temperature signal at input linearly.

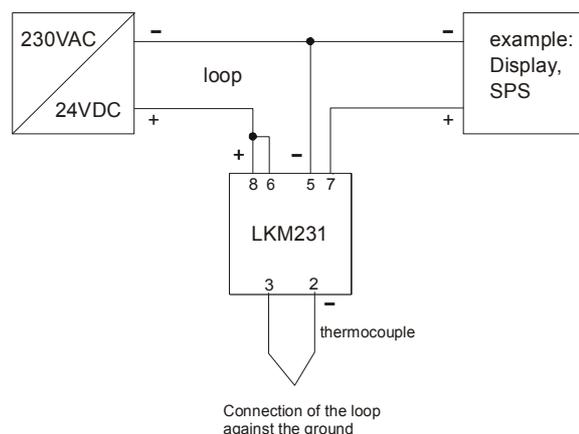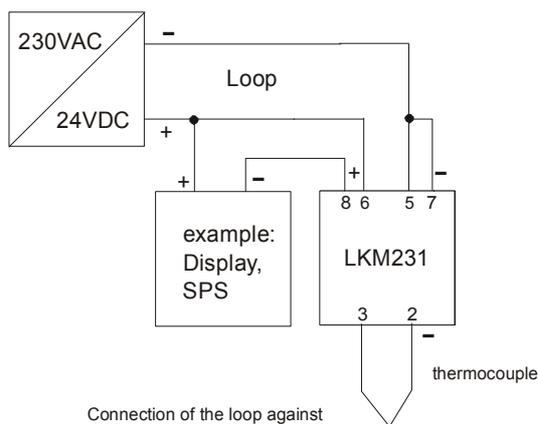

## DEBUGGING AND CORRECTION

A thermocouple supplies a voltage signal that is proportional to the temperature difference between the measurement location and the reference junction, i.e. the thermocouple does not supply a voltage if the measured temperature is equal to the reference junction temperature. In the event of a short circuit of the thermocouple or the compensating lead the new measurement location is sited at the place where the short circuit occurs.

<b>Fault observed</b>	<b>Cause of the fault</b>
No current in the loop	No supply voltage Incorrect polarity Defective Display unit Lead fractured
Output signal corresponds to room temperature	Short circuit in sensing element
Output signal >20 mA	Sensing element fractured
Absolute value in the display looks correct, but it has a negative sign	Polarity reversed on the evaluation unit
If the measurement location is heated up the output signal reduces	Thermocouple polarity incorrect
Display obviously too high or too low	Incorrect compensating lead or connected up with polarity reversed Incorrect thermocouple
When only one pole of the couple is clamped up a value is still displayed	Electromagnetic disturbances are coupled into the input lead

Subject to modifications arising from errors or technical advancements



August 2011

